



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

Alztal-Alpakas/Hermann Gröbner
Feldkirchner Str. 1
Trostberg 83308 Germany

07/30/15

Test No: 908785


Animal and Sample Description

Animal Name: Appy Bernardo
Breed: Alpaca(Huacaya)
Sex: Male
Color: Multi

Animal ID: 276093400560136
Sample Location: Side (L)
Sample Date: 05/23/15
Age: 10/26/14

Laboratory Data

Mean Fiber Diameter:	20.3 microns	Spin Fineness:	20.1 microns
Standard Deviation:	4.7 microns	Mean Curvature (deg/mm):	35.2
Coefficient of Variation:	23.2 %	SD Curvature (deg/mm):	21.9
Fibers Greater Than 30 microns:	2.0 %	Comfort Factor:	98.0 %

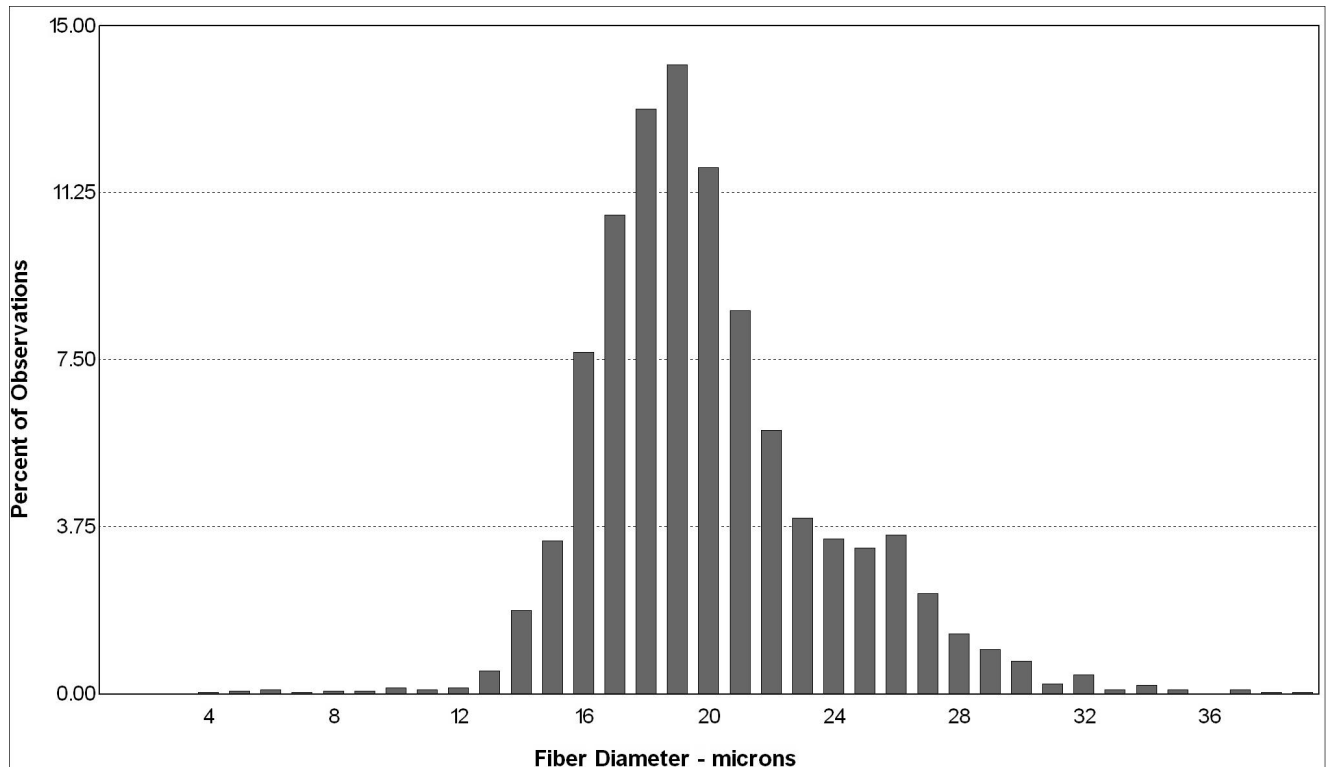

This Test Performed According to I.W.T.O Method 47